

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

OCT 28 2009

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N <u>130493</u>
Name <u>J. Swartz</u>		ID# <u>4314</u> Date <u>2/28/09</u>
A	Agency <u>SCDL</u>	Phone # <u>269-5592</u>
Instrument Location <u>SCDL</u>		
Alco S/N <u>SC07108</u>		Target Value <u>.080</u> High Pressure <u>900 psi</u>
B	Alco Test Values <u>.076</u> <u>.077</u> 1 st Alco 2 nd Alco	
Signature <u>[Signature]</u>		<u>CBS</u> <u>10/24/09</u>
(OVER)		

(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

Nita J. Bolz
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 9th day of Nov., 2009.

[Signature]
Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office

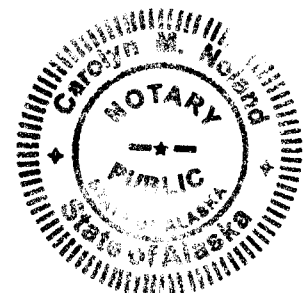

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130493

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

Breath Test Record

Serial Number 130493 Model DataMaster
Location CLR4 Clear Air Force Station

Subject Information

Last Name Verification Of Cal O.L. # L
First Name L

Operator Information

Operator Name Swartz/J Case
Operator # 4314 Department AAA1

Test Results

Alco Target .080 Alco Serial SCOTT08
Nominal 0.08 Barometer 30.07 Test Type V
Dry Gas 1 0.076 Time: 23:51:46 Test Date 02/28/2009
Subject Alcohol 0.000 Time: 23:53:49 Test Time 23:50:43
Dry Gas 2 0.077 Time: 23:54:48 Report Y

INTERNAL STANDARD
ALCO TV 30.07 in .076
BLANK TEST .000
SUBJECT SAMPLE .000
BLANK TEST .000
ALCO TV 30.07 in .077
BLANK TEST .000

8 2/28/09

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130493

FEBRUARY 28, 2009
TIME 23:48

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 01/08/09
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 41c
BAROMETER: 30.07 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEFGHIJ
KLMNOPQRSTUVWXYZ[\]^_`abcde fghijklmno
pqrstuvwxyz{|}~